



F305x Series

Handheld Dewpoint Meter

• Instruction Manual •

Version: 1.04

Experts in Compressed Air & Fluid Measurement

Fast · Accurate · Management

Preface

- Dear customer, thank you for choosing our products.
- This manual is a description of the use range, functions, installation and operation methods, troubleshooting, and maintenance of the product.
- The user must read this operation manual completely before using the device to properly use the product.
- After you read it, keep it in an accessible place for the next operational reference.

Notice

- Fix Instruments is not responsible for damage caused by unauthorized changes to the equipment without reviewing the operation manual or violating the provisions of this operation manual, and the instrument guarantee will be automatically voided.
- Fix Instruments is not responsible for incidental damage caused by transportation, equipment performance, or mishandling.
- Fix Instruments do not promise the suitability of this equipment for any application not described herein.
- Fix Instruments have tried to make the information in this manual correct. If you find any problems, you are welcome to contact us.
- The contents of this manual are forbidden to be reproduced, copied, or modified without permission.

Contents

Preface	3
Notice	3
1 Safety Instructions	5
1.1 General Safety Instructions	5
1.2 Storage and Transport Safety	5
2 Product Overview	7
2.1 Application	7
2.2 Features	7
2.3 Technical Data	7
3 Dimension & Installation	10
3.1 Dimension (in mm)	10
3.2 Packing List	11
3.3 Installation & Operation	11
3.4 UI Operation Guide	12
3.5 Setting Menu	14
3.6 File Export	15
4 Calibration & Maintenance	16
4.1 Sensor Module	16
4.2 Calibration	16
4.3 Maintenance	17
5 Warranty Terms	19
5.1 Warranty Period	19
5.2 Warranty Coverage	19
5.3 Warranty Certificate	19
5.4 Warranty Channels	19

1 Safety Instructions

1.1 General Safety Instructions

**Danger!****Compressed air!**

Any contact with rapid air leaks or pressurized parts of the compressed air system can lead to significant injury or even death.

- Never exceed the recommended pressure range.
- Make sure air tools & hoses are in good condition.
- Ensure the system is not under pressure when performing repair & maintenance.

**Danger!****Power voltage!**

Any contact with the electrical parts of the product can lead to significant injury or even death.

- Consider all electrical installation-related regulations.
- Any power connections must be disconnected when performing repair & maintenance.
- Any electrical work on the system is to be performed by authorized personnel only.

**Attention!****Operating conditions!**

Please check the permissible operating conditions. Any operation beyond these limits could potentially cause measurement failure or even damage the instrument or the entire system.

- Please review national standards and regulations during the preparation and installation process.
- The product is prohibited for use in explosive areas.
- Ensure the product operates within the allowed working conditions.

**Caution!****Product malfunction!**

Incorrect handling and improper transport could cause product malfunction.

- Unauthorized disassembly of the product is prohibited.
- Use correct and appropriate tools to operate to product.
- In case the product malfunctions, please stop using it and contact customer support.

1.2 Storage and Transport Safety

- Ensure the product is transported at a temperature of -10 ... +60 °C.
- It is recommended to use the product's original packaging for storage and transport.
- Make sure the product is stored at a temperature of -10 ... +60 °C.
- Avoid exposure to sunlight and UV rays.
- The storage humidity must be < 70% and free of condensation.

2 Product Overview

2.1 Application

The F305x handheld dewpoint meter is a handheld instrument that integrates dewpoint measurement, data analysis and recording. It is suitable for on-site inspection, working condition analysis and diagnosis, and can simultaneously measure temperature, pressure and humidity parameters.

Integrating FIXINST-P polymer film capacitive sensor and FIXINST-A ultra-fast response Al₂O₃ sensor with updated moisture-sensitive materials and processes, enabling F305x to accurately measure a wide range of dewpoint from -110 ... +60 °Ctd

The dewpoint curve prediction algorithm quickly and accurately predicts the final stable value and time required, thus efficiently complete on-site inspections. Curve sparse and data recording functions, real-time sparse dewpoint, temperature, pressure and other data measurement curves, record on-site working condition data, and easily analyze gas state change trends

The measurement chamber is equipped with a drying system that protects and dries the sensor when the instrument is not measuring, ensuring a quick response to the next measurement.

2.2 Features

- ✓ Compatible with various sensor technologies: polymer thin film, aluminum oxide sensors that can be used in different measurement ranges
- ✓ MEMS based pressure sensor for monitoring dewpoint and online pressure simultaneously (Abs. pressure 0 ... 1.7 MPa.a)
- ✓ Accurate to ± 2 °Ctd with up to 10+ dewpoint calibration and multi-point temperature compensation (Refer to **Technical Data**)
- ✓ Dewpoint steady-state prediction helps customers predict the trend in advance to save waiting time
- ✓ Data logging and graphing
- ✓ Equipped with a dry measuring chamber to ensure ultra-fast response and high accuracy
- ✓ Outstanding long-term stability
- ✓ 4.3" IPS wide viewing angle LCD with capacitive touch, data clearly displayed and user-friendly HMI
- ✓ Handheld so easy to use, start measurement by connecting the PTFE tube to the measuring chamber, no site restriction, no operational technical difficulties

2.3 Technical Data



Measuring Range	
Dewpoint	
F305A	-60 ... +60 °Ctd

F305B	-110 ... +60 °Ctd
Temperature	-40 ... +100 °C
Pressure	0 ... 1.7 MPa(a)
Accuracy	
Dewpoint (Air or Nitrogen)	
+20 ... -60 °Ctd	±2 °Ctd
-60 ... -100 °Ctd	±3 °Ctd
Temperature (Customizable)	
0 ... +50 °C	± 0.3 °C (Standard)
-40 ... 0 °C & +50 ... +100 °C	± 0.5 °C (Standard)
Pressure	
Accuracy @23°C	±0.3 %FS
Pressure Drift with Temperature	±0.001 MPa/10 °C
Response Time	
Dewpoint: 63% [90%], Reference: 20 °C, 1bar(a), 4L/min	
-50 → +20 °Ctd	20 sec [40 sec]
+20 → -50 °Ctd	1 min [3 min]
Pressure	< 1 sec
Power	
Battery Charging	PD fast charger, 20 VDC 1A
Charging Interface	Type-C interface
Charging Time	2.5 h
Battery Life	16 h (at 20 °C operating temperature)
Operating Environment	
Medium Temperature	-30 ... +70 °C
Operating Temperature	0 ... +50 °C
Storage Temperature	-10 ... +60 °C (Recommended +20 °C)
Relative Humidity	0 ... 95 %RH

Sample Gas Flow Rate	>2 L/min
Pressure	0 ... 1.7 MPa(a)
Output	
File Export	Type-C interface
Other	
Display	4.3" IPS LCD with capacitive touch
Data log	1.5 G storage, 200,000,000 values
Process connection	Dewpoint sensor: ISO G 1/2" thread Measuring chamber: 6 mm hose with fast connector

3 Dimension & Installation

3.1 Dimension (in mm)

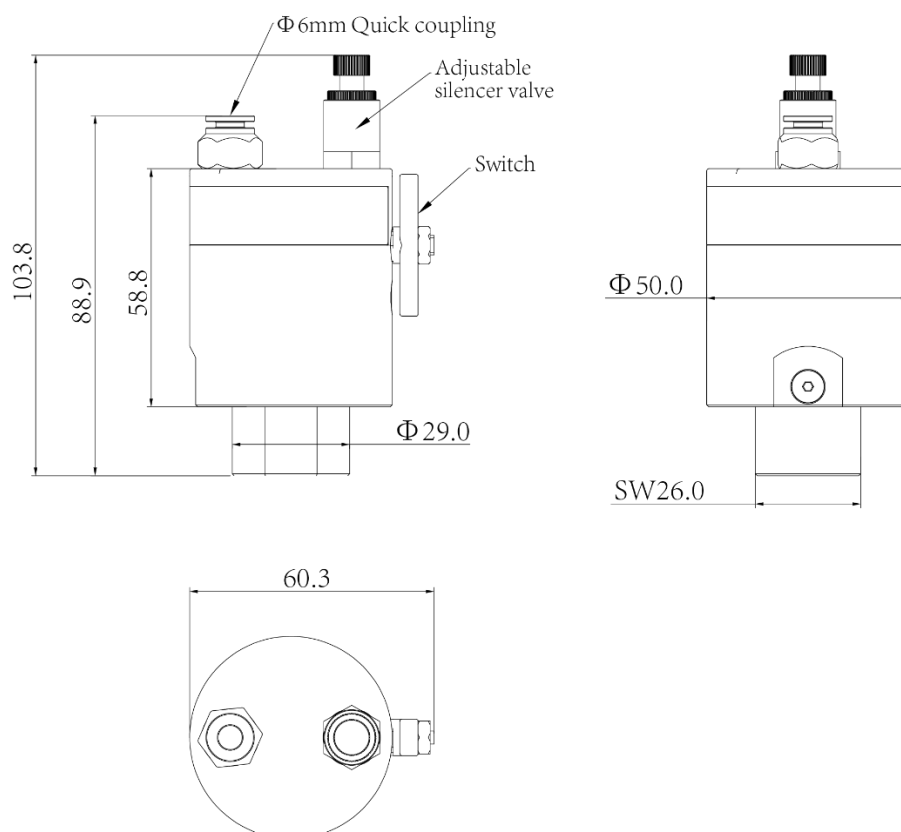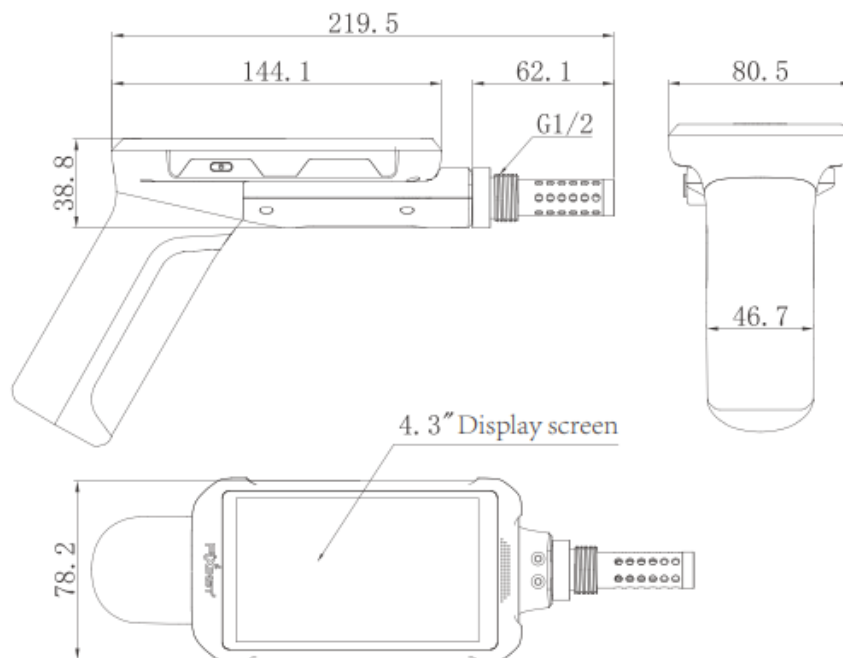

3.2 Packing List

No.	Description	Quantity
1	F305x Handheld dewpoint meter	1
2	Measuring chamber	1
3	Charger + Charging cable	1
4	Teflon tube (2m) + Male quick-connect coupling ($\phi 6\text{mm}$)	1
5	FixInst Online dewpoint meter connection kit (optional)	1
6	Female quick-connect coupling ($\phi 6\text{mm}$)	1
7	OTG Type-C USB flash drive	1
8	Reserve desiccant	1
9	Envelope (quick guide + calibration certificate)	1
10	Specialized portable protective case	1

3.3 Installation & Operation

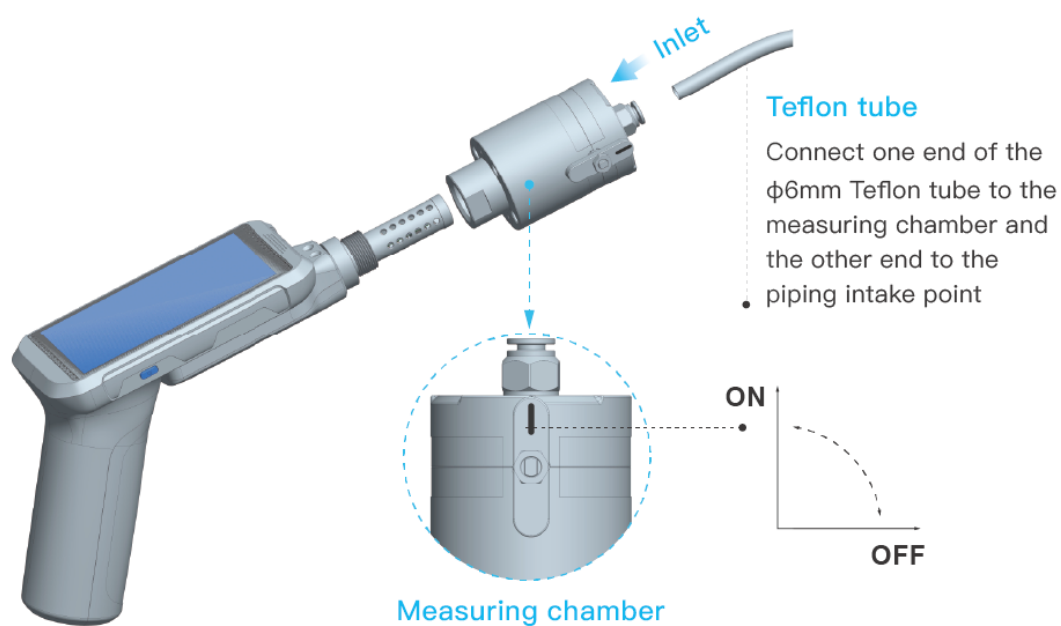


Figure 3-3 Measuring Chamber Usage Guide

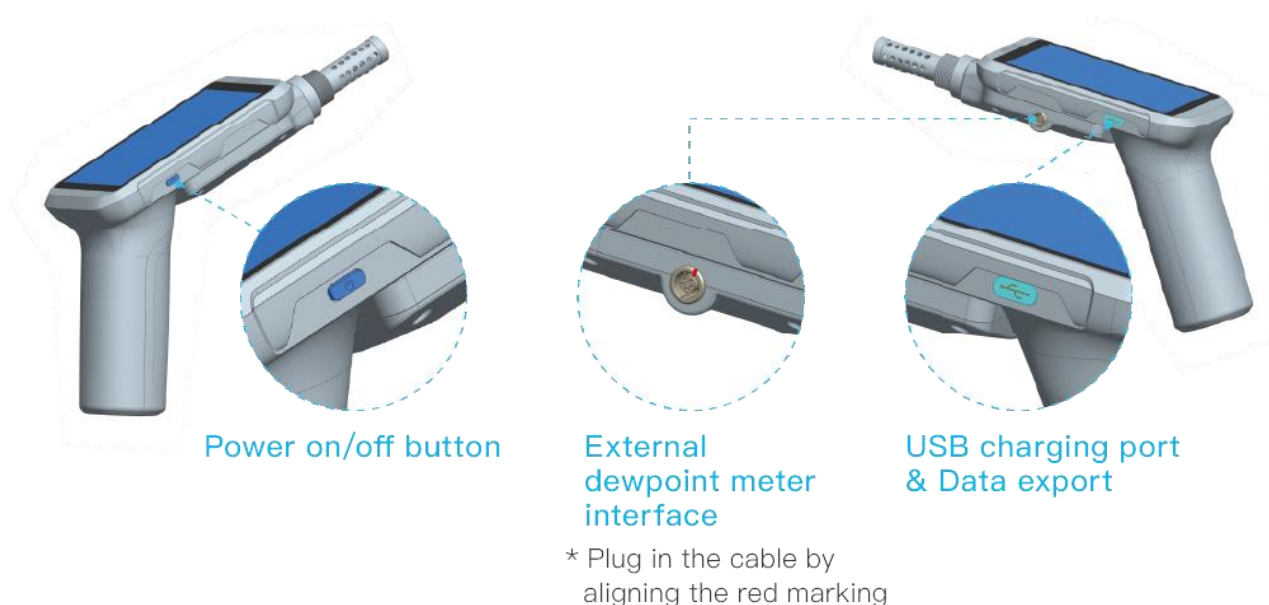


Figure 3-4 F305x Button Locations and Functions

3.4 UI Operation Guide

Due to software upgrade, the actual product interface may differ from the manual, the actual interface shall prevail. For technical support, you can contact FixInst after-sales service to get the latest operation guide (the following guide apply to software version V1.02).

- **UI-Value**

Predictive Dewpoint Value

This value indicates the final stabilized value of the dewpoint calculated by the algorithm

Display Channel Selection

Long press on the data line to customize the parameters to be presented


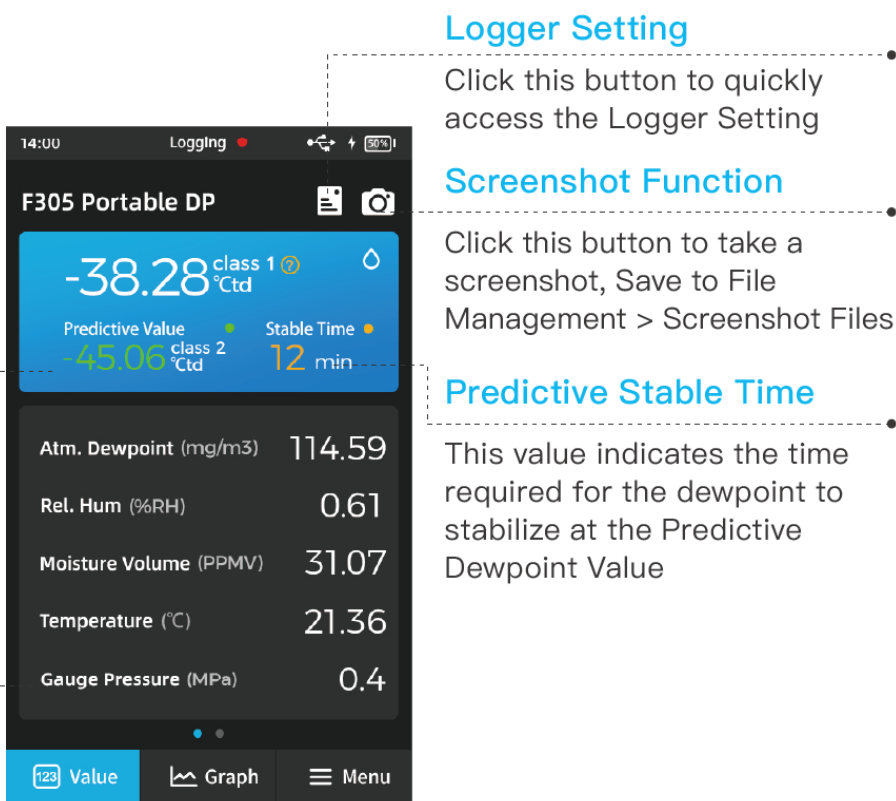


Figure 3-5 F305x Value Interface

• UI-Graph

Y-axis Selection

Click here to select the Y-axis parameter from the drop-down menu

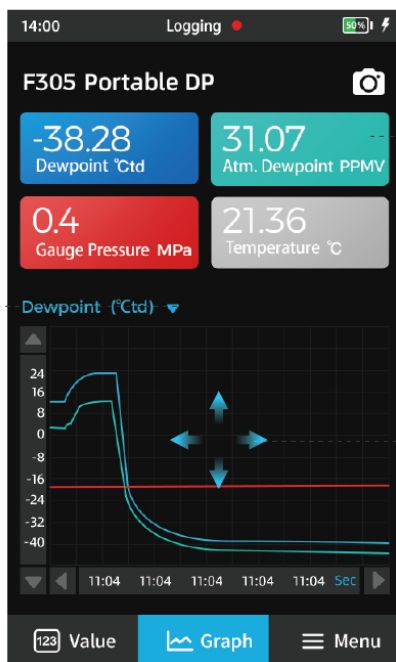

Curve Display

Clicking the button, the highlighted curve is displayed in the graph area. Clicking it again, the value turns gray and the curve is removed from graph

Data Curve Scaling

Within the coordinate area,
Two-finger horizontal scaling
adjusts the X-axis display area
Two-finger vertical scaling
adjusts the Y-axis display area

Figure 3-6 F305x Graph Interface

• UI-Setting

Data Logging

Data logging reminder function
Green dot flashes during data logging waiting
Red dot blinking during data logging

Sensor Setting


Click on this button to set the parameters of dewpoint, pressure, and temperature sensors

File Management

Click to view Screenshot Files and Record Files

System Setting

Set the system language and time, upgrade and restart the device

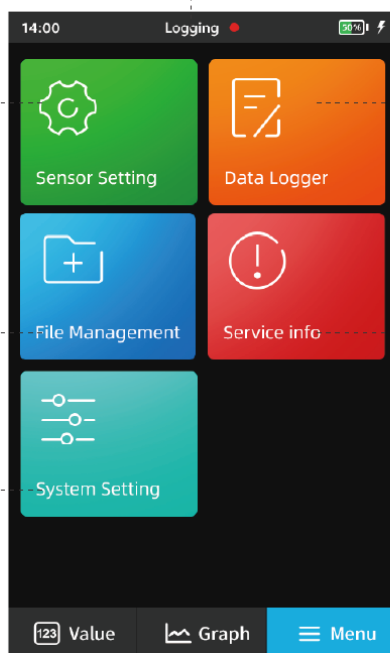

Data Logger

Click for data logging settings and related operations


Service Info

Click here to see supplier information and service information

Figure 3-7 F305x Setting Interface

3.5 Setting Menu

Note: Menus and content may be updated due to software upgrades, subject to availability or consult FixInst technical support.

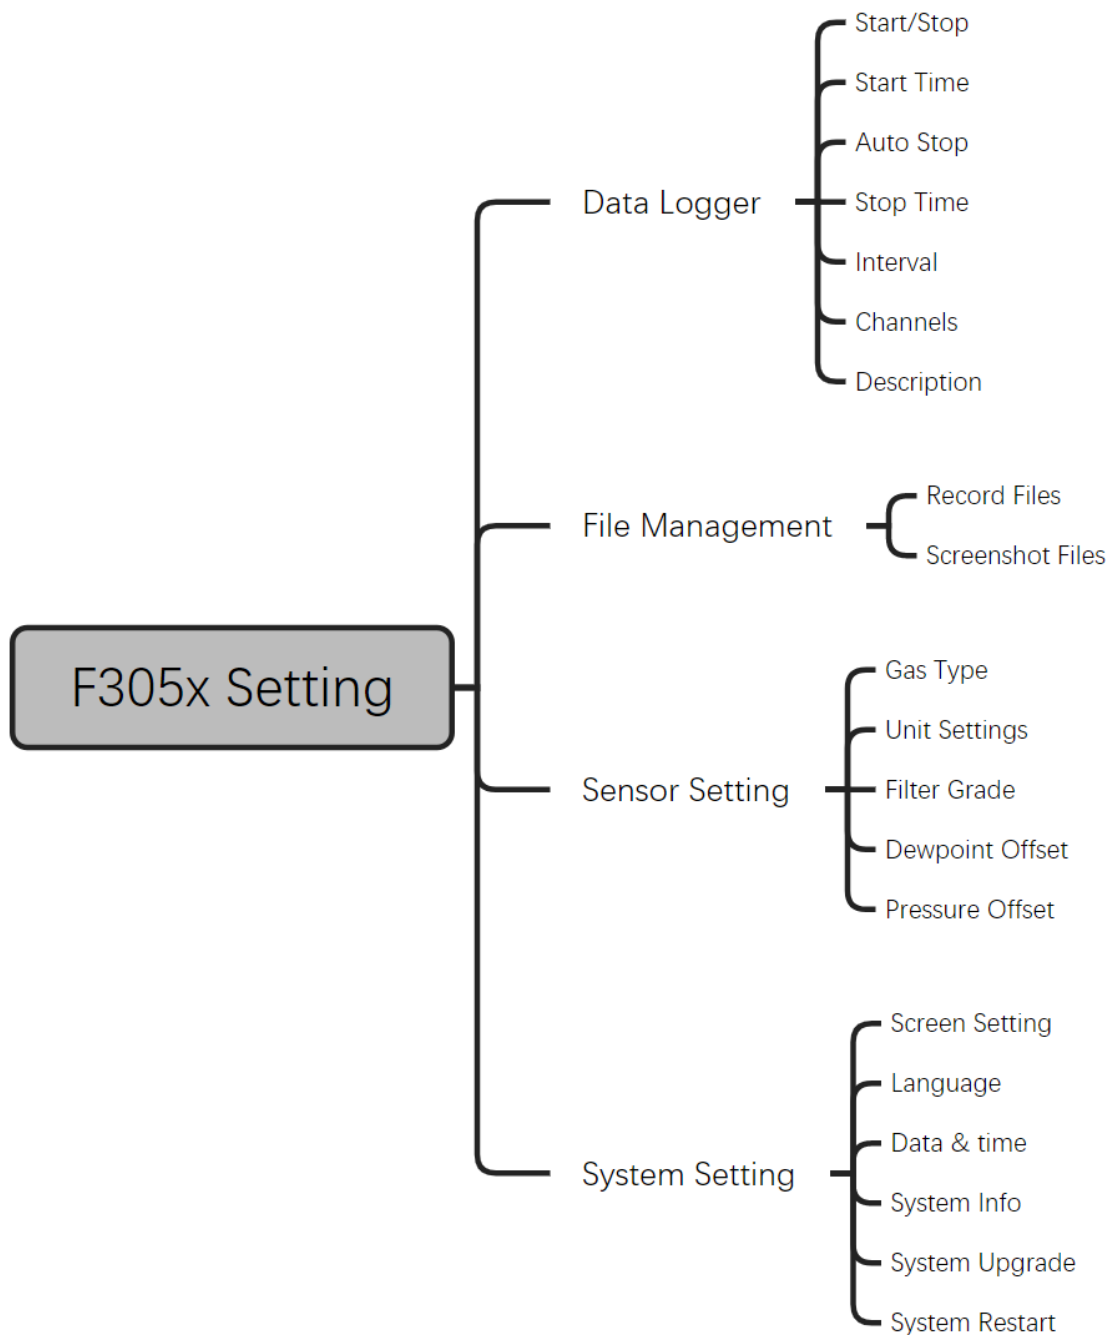

Data Logger:

Function Name	Function Description
Start/Stop	Click to start or stop data logging.
Start Time	Set the Start Time for logging, defaults to the current time but supports setting a scheduled start time.
Auto Stop	Set whether the logging stops automatically.

Stop Time	When Auto Stop function is enabled, set the stop time, defaults to start time + 8 hours.
Interval	Set the interval time for logging measurement values.
Channels	Select measurement channels.
Description	Enter description for this data logging.

File Management:

Function Name	Function Description
Record Files	Display all Record Files saved by the device, with options for export and delete.
Screenshot Files	Display all Screenshot Files saved by the device, with options for export and delete.

Sensor Setting:

Function Name	Function Description
Gas Type	Set the type of medium being measured.
Unit Settings	Set the Pressure Unit and Temperature Unit.
Filter Grade	Set the sensor filtering grade to adjust the sensor sensitivity.
Dewpoint Offset	Perform single-point calibration for dewpoint value.
Pressure Offset	Perform single-point calibration for pressure value.

System Setting:

Function Name	Function Description
Screen Setting	Set Screen Brightness. Set Off-screen.
Language	Set system language: Simplified Chinese / Traditional Chinese / English.
Data & time	Set Current date & time.
System Info	Display Sensor Information, Display Information, CPU Temperature, and other product information.
System Upgrade	Insert the flash drive to update device firmware.
System Restart	Restart the device.

3.6 File Export

After inserting the USB drive, access **Menu > File Management > Record Files/Screenshot Files**, select the files/screenshots to export, and click **Export**. The exported files will be saved to the USB drive in CSV (record files) and PNG (screenshot files) formats.

4 Calibration & Maintenance

4.1 Sensor Module

If calibration & maintenance of the sensor module are required, please follow the steps below to uninstall/install the sensor module:

Step1.

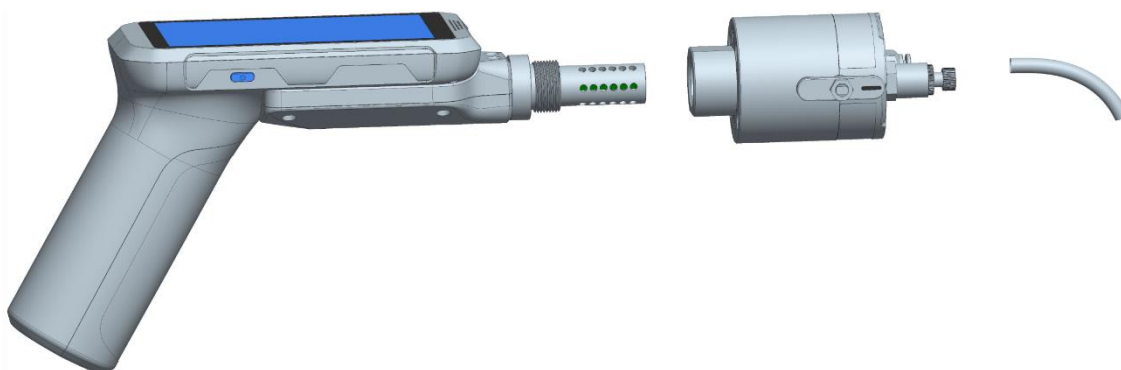


Figure 4-1 F305x Uninstall/Install Sensor

Step2.

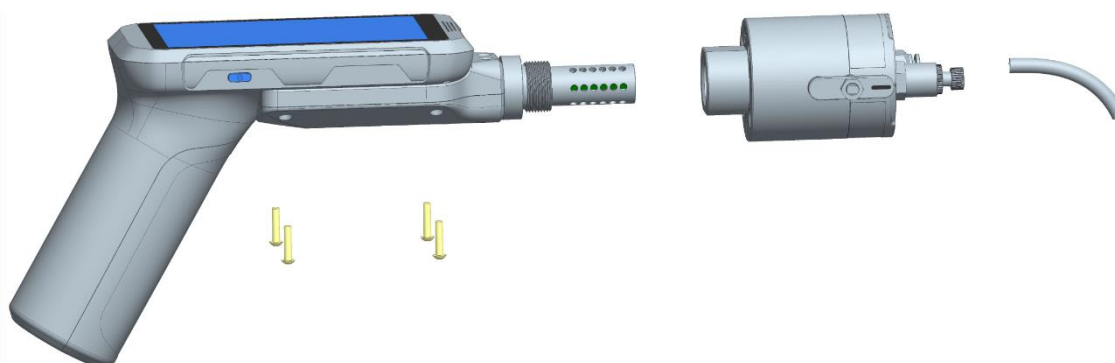


Figure 4-2 F305x Uninstall/Install Sensor

Step3.

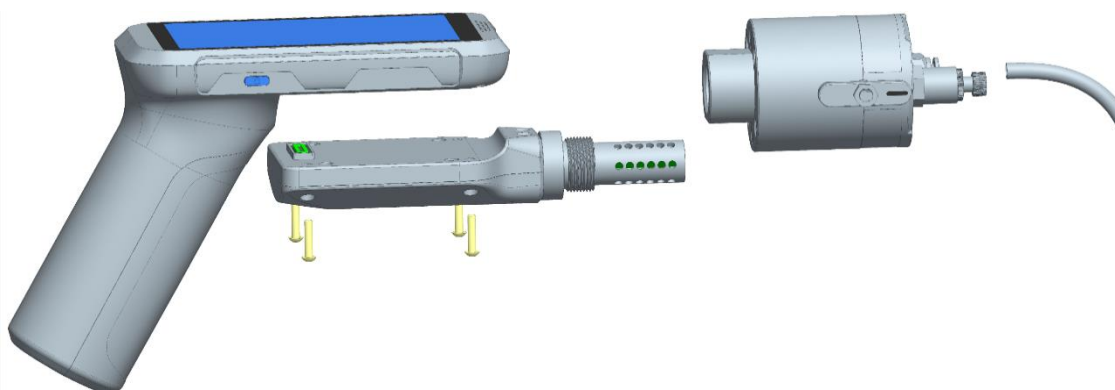


Figure 4-3 F305x Uninstall/Install Sensor


4.2 Calibration

The product is factory calibrated and the calibration certificate is attached to the product.

Since the measurement accuracy of the product is affected by the on-site environment (oil, high humidity, or other impurities can affect the accuracy), we recommend the user perform calibration once a year.

Calibration service is not covered by the product guarantee. Please contact the manufacturer in case calibration is required.

FAST
ACCURATE
MANAGING



www.fix-instruments.com

MEASUREMENT
EXPERT
SPECIALIZES
IN COMPRESSED AIR & GAS

CALIBRATION CERTIFICATE

Instrument F133C

Series number 1138501030001

Manufacturer Fix Instruments

Calibration date 30 Aug 2018

CALIBRATION RESULTS:

Description	Units	Reference value	Measured value	Evaluation
Dew point	°Ctd	19.82	19.32	Passed
		9.74	8.94	Passed
		-0.42	-0.72	Passed
		-10.60	-10.90	Passed
		-20.12	-20.42	Passed
		-30.58	-31.18	Passed
		-40.10	-40.40	Passed
		-50.38	-50.48	Passed
		-60.08	-61.08	Passed
		-70.04	-70.74	Passed
Temperature	°C	5.00	5.00	Passed
		25.00	25.00	Passed
		35.00	35.00	Passed
Pressure	bar(a)	0	0	Passed
		3.00	3.00	Passed
		9.00	9.00	Passed


EQUIPMENT USED IN CALIBRATION:

Type	Serial number	Uncertainty
MBW 373LX	16-0431	±0.1 °C
PT100	JD170504170	±0.1 °C
P3000	18083000790	±0.012 bar

Ambient condition: Humidity 30...60 %RH / Temperature 20...26 C / Pressure 1015±20 hPa / Flow 2...4 L/min

Modbus RTU setting: Address: 1 / Baudrate: 9600 / Framing: Parity, Stop bit: 8, None, 1

The above instruments was calibrated by comparing the dewpoint output to MBW 373 LX dewpoint mirror in the Fix Instruments Humidity Calibration Laboratory. The calibration is according to FixInst working standard and traceability chain for dew point, temperature and pressure calibrations.

Checked By 

This report is the test result of FixInst laboratory, it is real and effective

Figure 4-4 Dewpoint Calibration Certificate (for Reference Only)

4.3 Maintenance

Please check the measuring chamber regularly. If contamination or blockage is found, please contact the manufacturer and clean the measuring chamber under their guidance.

**Caution!**

- **Wet or contaminated sensor will result in longer response time or even incorrect measurement result.**
- **Do not touch the sensor directly.**

5 Warranty Terms

Dear Customer:

Thank you for choosing FixInst products. We have always been committed to providing our customers with high-quality, high-performance instrumentation products to meet your needs in a variety of application scenarios.

In order to ensure your satisfaction after purchasing the product, please read the following after-sales terms and conditions carefully, so that you can correctly and efficiently apply for the warranty service when needed.

5.1 Warranty Period

12 months from product shipment.

5.2 Warranty Coverage

1、Warranty period due to the product's own problems caused by performance failures, confirmed by the seller's test, will provide free maintenance services; human misuse or due to the site of the product working conditions and the product type does not match the damage caused by the exceptions.

The following are not covered by warranty:

- ① Product damage caused by force majeure factors (such as natural disasters, etc.).
- ② Products due to natural wear and tear, rough handling caused by the appearance of damage, scratches or wear (such as impact caused by the loss of paint, surface bumps, etc.).
- ③ Damage caused by disassembling the product without the Company's consent or unauthorized changes in the use of the product.
- ④ Damage to the product caused by repair or modification not authorized by the company.
- ⑤ Damage caused by improper use of the product by the user or operation in violation of the instructions.
- ⑥ Products purchased from unauthorized sources.

2、For non-warranty or non-warranty product failure, we will provide paid repair services, the specific cost depends on the actual situation.

5.3 Warranty Certificate

Users are required to provide valid proof of purchase (e.g., invoice, receipt, etc.) and product serial number when applying for warranty service.

5.4 Warranty Channels

Users can apply for after-sales warranty service by filling out our after-sales treasure system or contacting customer service personnel.

<https://www.fix-instruments.com/h-col-143.html>

Experts in Compressed Air &
Fluid Measurement

Fix Instruments (Shenzhen) Co., Ltd.

A: 2/F,Middle Block, Building B, TG Science Park, No. 2 LuoZu Industrial Avenue,
ShiYan Subdistrict, Baoan District, Shenzhen, GuangDong, China

M: sales@fix-instruments.com

P: 0755-2359-1123

